



## INTENDED USE OF SURGICAL KIT COMPONENTS


### OPTIONS FOR REMOVING IMPLANT FROM CONTAINER AND PLACING IN OSTEOTOMY

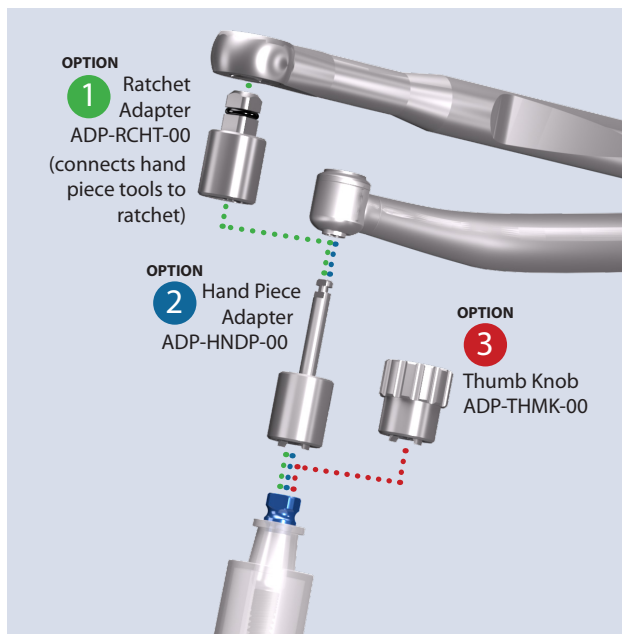

### OPTIONS FOR DRIVING IMPLANT TO FULL DEPTH

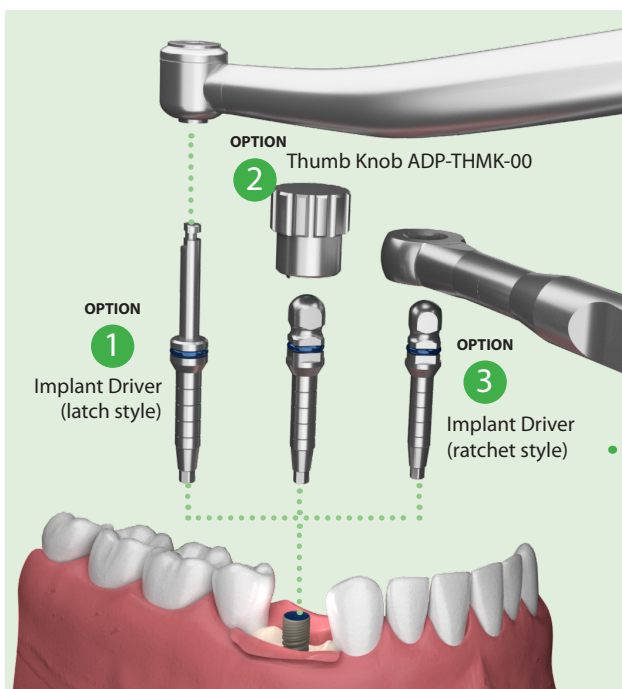

### OPTIONS FOR REMOVING CARRIER FROM IMPLANT

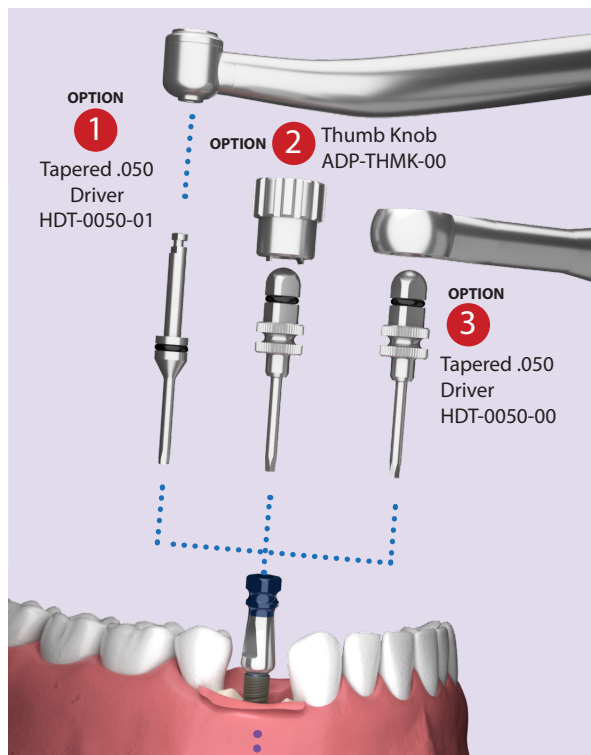

**Do not drive implant to full depth with the carrier – it may damage the hex connection inside the implant.**

**Use one of these options to finish the installation after the implant is stabilized.**